

## FLX-96 Plate

Handling guide for FLEXcyte 96 (FLX-96) plates used for contractility assays with human iPSC-derived cardiomyocytes.





# TOC

1. Introduction.....	4
2. Workflow .....	5
3. Day 0 - Handling of FLX-96 plates upon arrival and before use .....	6
3.1 Important hints upon arrival of FLX-96 plates.....	6
3.2 Preparation of FLX-96 plates before use .....	7
4. Day 0 - FLX-96 plate coating with fibronectin .....	8
4.1 Supplementary material for FLX-96 plate coating .....	8
4.2 Procedure.....	9
5. Day 0 - Seeding of hiPSC-derived cardiomyocytes into FLX-96 plates .....	9
5.1 Important hints before seeding of FLX-96 plates .....	9
5.2 Supplementary material for FLX-96 plate seeding.....	10
5.3 Procedure.....	12
6. Day 1 – approx. Day 5 - Medium exchange of FLX-96 plates.....	12
6.1 Important hints before medium exchange of FLX-96 plates.....	12
6.2 Supplementary material for FLX-96 plate medium exchange.....	13
6.3 Procedure.....	14
7. Day 5 - Day 7 - Compound addition and analysis .....	15
7.1 Important hints before compound addition to FLX-96 plates.....	15
7.2 Supplementary material for compound addition and analysis .....	16
7.3 Procedure.....	17
8. Appendix .....	18





## 1. Introduction

The FLEXcyte 96 (FLX-96) plates are designed for high-throughput cardiac contractility measurements using the FLEXcyte 96 system, an add-on system for the CardioExcyte 96 device provided by Nanion Technologies.

FLX-96 plates are ready-to-use and should always be handled with care. Each of the wells contains a flexible membrane as substrate for the cells, disruption of the membrane will eliminate the well from performance in the FLEXcyte 96 system. Please read the entire user guide before you start your experiment and contact [info@innovitro.de](mailto:info@innovitro.de) in case of questions regarding handling of the FLX-96 plate or [support.cellular.networks@nanion.de](mailto:support.cellular.networks@nanion.de) for questions regarding the FLEXcyte 96 software.

The cardiomyocytes used for FLX-96 plates are from human induced pluripotent stem cell (iPSC)-derived origin and can be purchased by a variety of stem cell manufacturers. According to the manufacturer, differences in cell handling may occur (e.g. cryopreserved or pre-cultured cells upon delivery, medium or cell numbers for seeding). Please read the manufacturer's cell handling guide carefully before you start your experiment with the FLX-96 plate.

Depending on the aim of the experiment, a serum-free buffer may be needed for compound addition, e.g. when positive inotropic effects of cardiomyocytes are the main interest. A validated serum-free buffer can be purchased with the FLX-96 plates from innoVITRO.


Helpful clues for every step are provided at the beginning of each chapter, read these hints carefully to obtain optimal results with FLX-96 plates.

You will find a PDF and a video version of this Handling Guide on [www.innovitro.de](http://www.innovitro.de).





## 2. Workflow

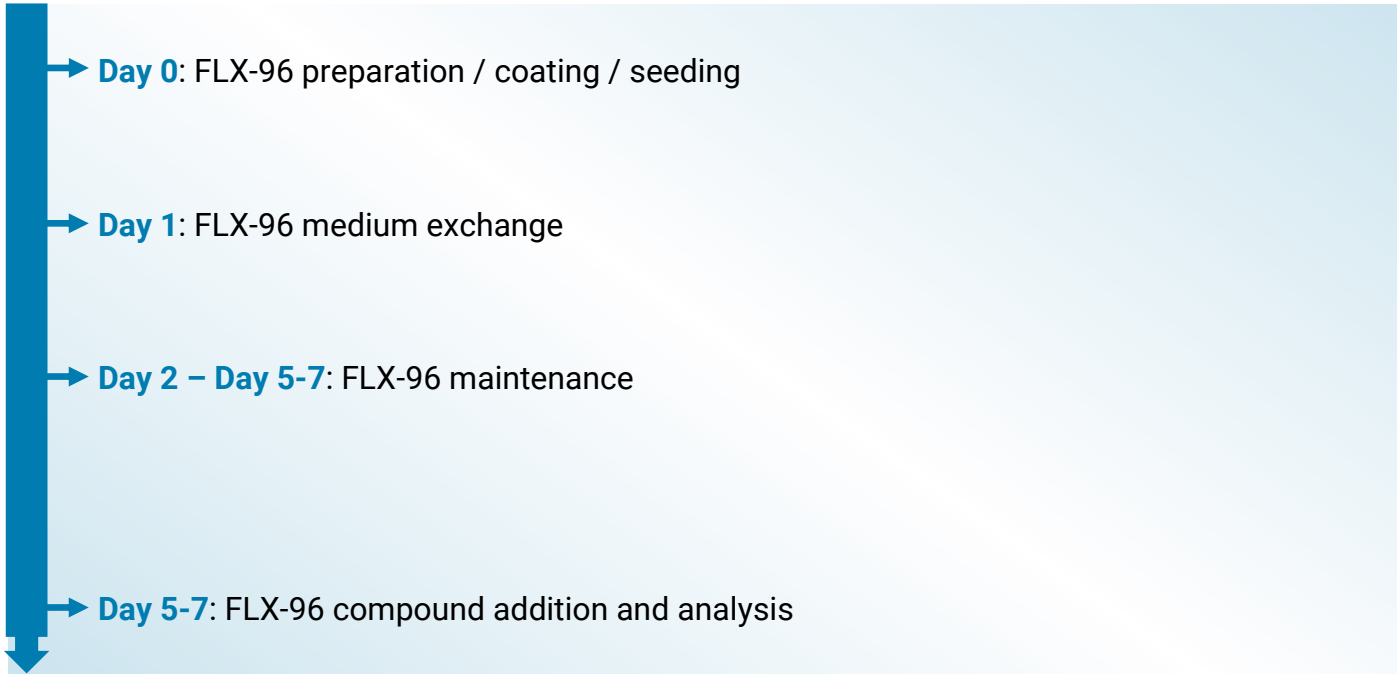

### Notes

---

---

---

---

---

---

---

---

---

---






### 3. Day 0 - Handling of FLX-96 plates upon arrival and before use

#### 3.1 Important hints upon arrival of FLX-96 plates


- FLX-96 plates are sterile and covered in vacuum-sealed plastic upon arrival. Please transport the sealed FLX-96 plate to a sterile environment (e.g. laminar flow hood) before removal of the plastic to avoid contamination before use. If the plates are not used straight away, do not remove the vacuum-sealed plastic and store the plates in a dry and dark environment at room temperature.
- The bottom of each FLX-96 well is covered with a very thin membrane which may be damaged if touched from inside or outside. Upon arrival, the FLX-96 plate is protected from above with a regular 96 plate lid and from below with a blue membrane protector. Before you start your experiment, make sure to exchange the blue membrane protector with a regular 96 plate lid (additionally provided with the FLX-96 plate). See step 3.2 (Preparation of FLX-96 plates before use) for detailed description how to handle FLX-96 plates upon arrival.

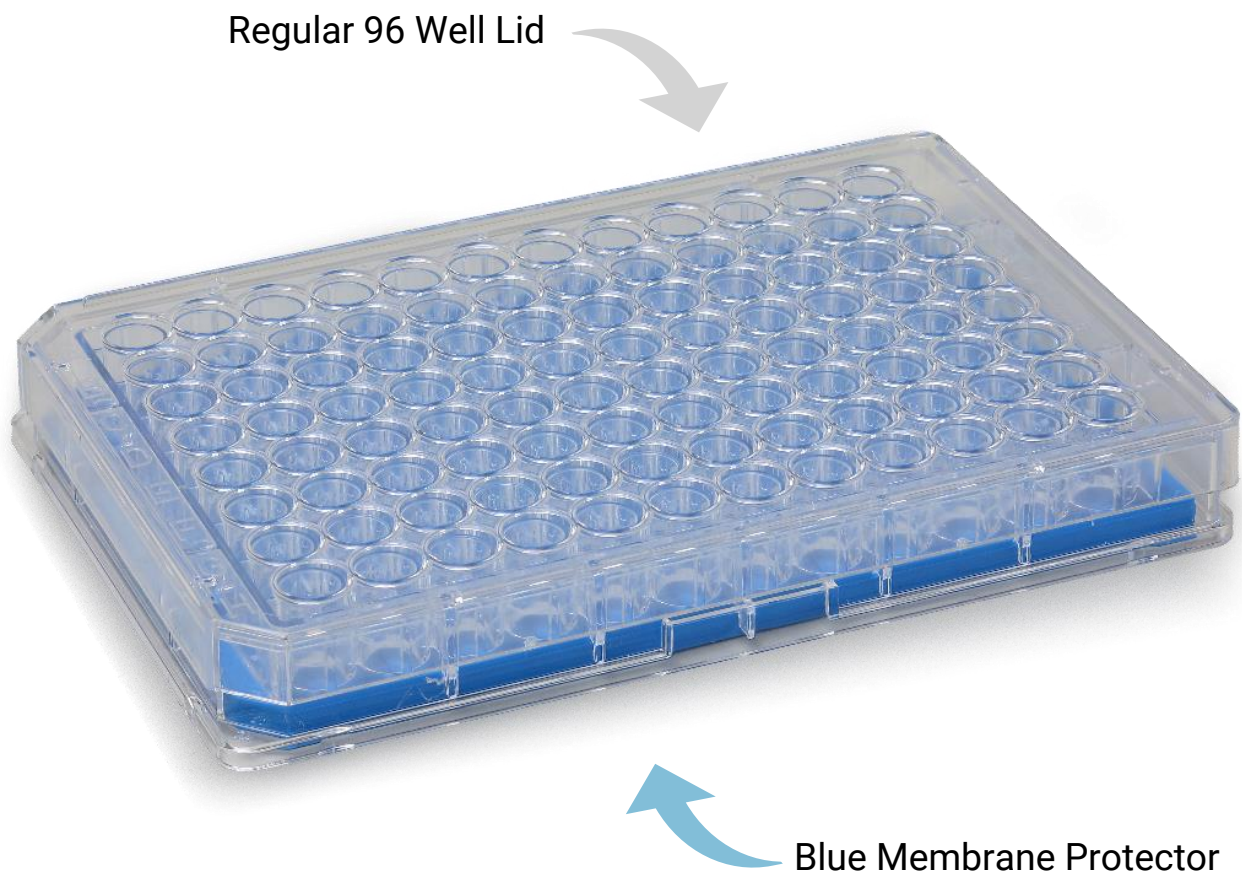



## 3.2 Preparation of FLX-96 plates before use

1. Transport the sterile and vacuum-sealed FLX-96 plate into a sterile environment, e.g. a laminar flow hood.
2. Unpack the additionally supplied lid and place it on a flat surface.
3. Open the vacuum-sealed packaging and remove it from the FLX-96 plate.
4. Put the FLX-96 plate together with the membrane protector on a flat surface.
5. Break the banderole and carefully lift the FLX-96 plate together with the upper lid (green arrow) while holding the membrane protector (purple arrow) down at the remains of the banderole.
6. Place the FLX-96 plate upon the additional lid by stacking the plate onto the lid. Do not turn the lid upside down to avoid disruption of the membranes. Keep the FLX-96 plate stack onto the lid until measurements are performed in the FLEXcyte 96 device. (Approx. 5-7 days after seeding).

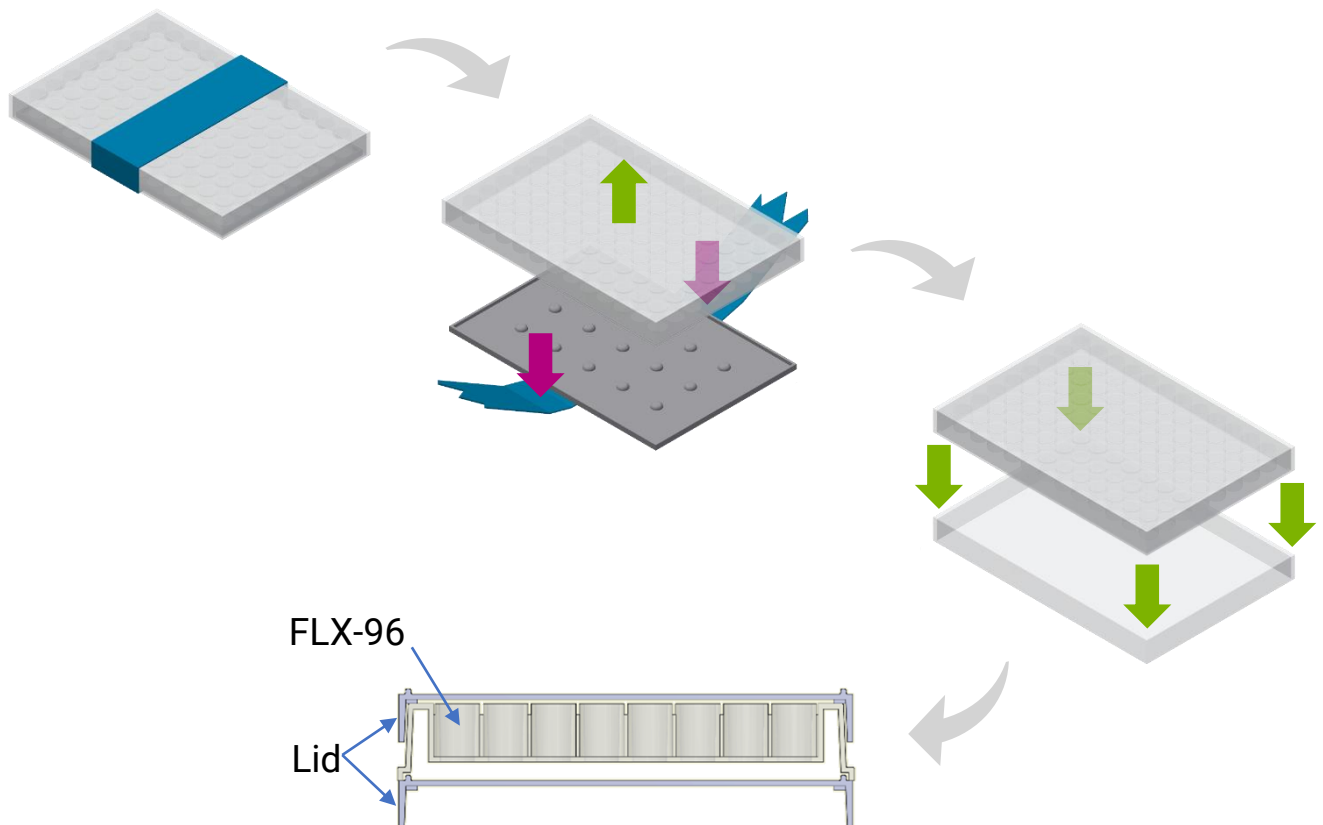



## 4. Day 0 - FLX-96 plate coating with fibronectin

### 4.1 Supplementary material for FLX-96 plate coating

#### Reagents:

- Fibronectin stock solution (1 mg/mL, e.g. Sigma Aldrich F1141)
- DPBS with Ca<sup>2+</sup> and Mg<sup>2+</sup> (e.g. GE Healthcare HyClone SH304264.01)
- Complete culture medium (optional: plating medium, please check cell manufacturer's guidelines before you start)

#### Disposable:

- FLX-96 plates
- Centrifuge tubes (50 mL)
- Serological pipettes (25mL)
- Reagent reservoirs (Integra CAT 4311)
- Pipette tips (1000 µL & 1250 µL)

#### Devices:

- Laminar flow hood
- Single channel adjustable pipette (e.g. 100-1000 µL)
- 12-channel adjustable pipette (100-1250 µL)
- Centrifuge (50 mL tubes)
- Water bath (37 °C)
- Incubator (37 °C, 5% CO<sub>2</sub>)
- Vacuum aspiration system
- *Optional: VIAFLO ASSIST (Integra 4500)*

*VIAFLO 12 Channel Pipette (Integra 4634)*







## 4.2 Procedure

1. Prepare 11 mL fibronectin coating solution in a sterile centrifuge tube by diluting 110  $\mu$ L fibronectin stock solution (1 mg/mL) in 11 mL of DPBS with  $\text{Ca}^{2+}$  and  $\text{Mg}^{2+}$ , resulting in a 10  $\mu$ g/mL fibronectin working solution. Mix the solution carefully.
2. Transfer the coating solution into a sterile reagent reservoir. Pipette 100  $\mu$ L of the coating solution to each well of the FLEXcyte Plate using a 12-channel pipette.
  2. (optional) When using a VIAFLO ASSIST with a 12-channel pipette, transfer the coating solution into a sterile reagent reservoir placed in the VIAFLO ASSIST, use program "ADD100 $\mu$ L" and start the coating procedure.
3. Place the lid back on to the FLX-96 and incubate the plate for 3 h at 37 °C.

## 5. Day 0 - Seeding of hiPSC-derived cardiomyocytes into FLX-96 plates

### 5.1 Important hints before seeding of FLX-96 plates

- Cells may be purchased cryopreserved or pre-cultured depending on the manufacturer. Different media for seeding or compound addition may also be provided by the manufacturer. Please read the cell manufacturer instructions carefully and follow recommendations for cell handling to ensure an optimal performance of the cells on the FLX-96 plate.
- According to your choice of stem cell manufacturer, different seeding densities of cardiomyocytes are required to achieve a synchronically beating syncytium. Please refer to table 1 for seeding densities according to your chosen commercially available cardiomyocyte.
- We recommend a manual counting chamber for consistent cell counting results.
- Depending on the number of compounds tested per FLX-96 plate, you may not need to seed the entire FLX-96 plate.

### Notes

---

---





## 5.2 Supplementary material for FLX-96 plate seeding

### Reagents:

- Complete culture medium (provided by cell manufacturer)
- Plating medium (only when recommended and provided by cell manufacturer)
- hiPSC-derived cardiomyocytes (cryopreserved or pre-seeded)

### Disposables:

- Fibronectin-coated FLEXcyte 96 plate (from Step 4.1)
- Centrifuge tubes (50 mL)
- Reagent reservoir
- Pipette tips (1000  $\mu$ L & 1250  $\mu$ L)

### Devices:

- Laminar flow hood
- Single channel adjustable pipette (e.g. 100-1000  $\mu$ L)
- 12-channel adjustable pipette (100-1250  $\mu$ L)
- Centrifuge (50 mL tubes)
- Water bath (37 °C)
- Incubator (37 °C, 5% CO<sub>2</sub>)
- Vacuum aspiration system
- *Optional: VIAFLO ASSIST (Integra 4500)*

*VIAFLO 12 Channel Pipette (Integra 4634)*

### Notes

---

---







## 5.3 Procedure

1. Thaw the cells according to manufacturer's guidelines.
2. Count the cells with a manual counting chamber and adjust the cells according to Table 1 (right column).
3. Transfer the cell suspension (11mL total) into a sterile reagent reservoir.
4. Remove the fibronectin solution from the wells with a vacuum aspiration system.
5. Pipette 100  $\mu$ L of the cell suspension to each well of the FLX-96 plate using a 12-channel pipette.  
*5.(optional) When using a VIAFLO ASSIST with a 12-channel pipette, transfer the cell suspension into a sterile reagent reservoir placed in the ViaFLO Assist, use program "CELLS\_ADD100 $\mu$ L" and start the seeding procedure.*
6. Immediately after cell seeding, transfer the FLX-96 plate into the incubator and let the cells settle over night.

## 6. Day 1 – approx. Day 5 - Medium exchange of FLX-96 plates

### 6.1 Important hints before medium exchange of FLX-96 plates

- We recommend a complete medium exchange with complete culture medium 18-24h after seeding.
- When medium change is performed manually: Remove the medium carefully row-wise with a single channel vacuum aspiration system. Four rows can be aspirated at a time before adding fresh medium. Do not remove the medium of the entire FLX-96 plate at once before adding fresh medium to avoid drying of the cells. Leave the FLX-96 plate on a flat surface when adding fresh medium and hold the 12-channel pipette in a 45° angle to avoid direct stress for the cell layer.
- When medium change is performed automatically with a pipette robot (e.g. INTEGRA VIAFLO ASSIST): The medium change can be performed at once for the entire plate, due to the high speed of the pipette robot the cells will not dry out during the procedure.
- After medium change, each well should contain a final volume of 200  $\mu$ L.
- Recommendations regarding the number of medium changes per week should be obtained from the respective cell manufacturer.





## 6.2 Supplementary material for FLX-96 plate medium exchange

### Reagents:

- Minimum of 22 mL complete culture medium

### Disposables:

- Serological pipette (e.g. 25 mL)
- Pipette tips (1250 µL)
- Reagent reservoir

### Devices:

- Laminar flow hood
- 12-channel pipette (100-1250 µL)
- Water bath (37 °C)
- Incubator (37 °C, 5% CO<sub>2</sub>)
- *Optional: VIAFLO ASSIST (Integra 4500)*  
*VIAFLO 12 Channel Pipette (Integra 4634)*

### Notes

---

---

---

---

---

---

---

---

---

---





## 6.3 Procedure

1. 18-24 h after seeding, warm at least 22 mL of complete culture medium for one FLX-96 plate.
2. Transfer the warm medium into a sterile reagent reservoir.
3. Aspirate the medium carefully with a single channel vacuum aspiration system to avoid disruption of the cell layer or membrane. Hold the FLX-96 plate in a 45° angle and aspirate four rows of the FLX-96 plate (A-H).  
*3. (optional) When using a VIAFLO ASSIST with a 12-channel pipette, transfer the fresh medium into a sterile reagent reservoir and leave it right next to the VIAFLO ASSIST. Place an empty reagent reservoir in the VIAFLO ASSIST, use program "REMOVE100µL" and perform medium removal twice. Afterwards exchange the reagent reservoir containing the waste medium with the reagent reservoir containing the fresh medium and dispense the fresh medium with program "ADD100µL". Perform this step twice again to reach the final volume of 200µL per well. Skip step 4 and 5 and proceed with step 6.*
4. Dispense 200 µL into each well using a 12-channel pipette. Leave the FLX-96 plate on a flat surface and hold the 12-channel pipette in a 45° angle to avoid maximum stress for the cell layer.
5. Proceed with the next four rows of the FLX-96 plate (E – H) and repeat steps 3 and 4.
6. Immediately after medium exchange transfer the FLX-96 plate back into the incubator.

## Notes

---

---

---

---

---

---

---

---

---

---





## 7. Day 5 - Day 7 - Compound addition and analysis

### 7.1 Important hints before compound addition to FLX-96 plates.

- Perform a last medium change 4-6 h before starting your measurements to keep nutrition levels stable for best cardiomyocyte performance.
- If positive inotropic effects are the main focus, we recommend serum-free medium during compound measurements. Please equilibrate the serum-free medium with the cap slightly open over night in the incubator the DAY BEFORE compound addition.
- If long-term measurements are performed (max. 5 days), we recommend serum containing complete culture medium during compound measurements.
- Have your measurement plan ready, before you start your experiment. Use Figure 1. (see appendix) as 96 well plate design template to set up your compound analysis plan.
- Prepare compounds in a 4x concentrated manner. Compound addition is performed with  $\frac{1}{4}$  (50  $\mu$ L) of the total medium per well, hence the final concentration will dilute to 1x concentrated per well.
- Perform a baseline measurement of the FLX-96 plate in the FLEXcyte 96 device, right BEFORE you add the compounds. We recommend 3 sweeps for a good reference baseline.
- Compound addition should be performed quickly to avoid temperature decrease of the plate. When using a FLEXcyte 96 benchtop device: compound addition is performed in the device.

#### Notes

---

---

---

---

---

---





## 7.2 Supplementary material for compound addition and analysis

### Reagents:

- 22+ mL complete culture medium *or* serum-free medium for final medium change
- 6+ mL complete culture medium *or* serum-free medium for compound preparation
- Compounds for your analysis

### Disposables:

- Serological pipette (e.g. 25 mL)
- Pipette tips (1250 µL)
- Reagent reservoir
- 96 deep well plate (for compound preparation)

### Devices:

- Laminar flow hood
- FLEXcyte 96 device (Nanion Technologies)
- 12-channel pipette (100-1250 µL)
- Water bath (37 °C)
- Incubator (37 °C, 5% CO<sub>2</sub>)
- Vacuum aspiration system
- *Optional: VIAFLO ASSIST (Integra 4500)*  
*VIAFLO 12 Channel Pipette (Integra 4634)*

### Notes

---

---

---











## 8. Appendix

Figure 1. 96 well plate template

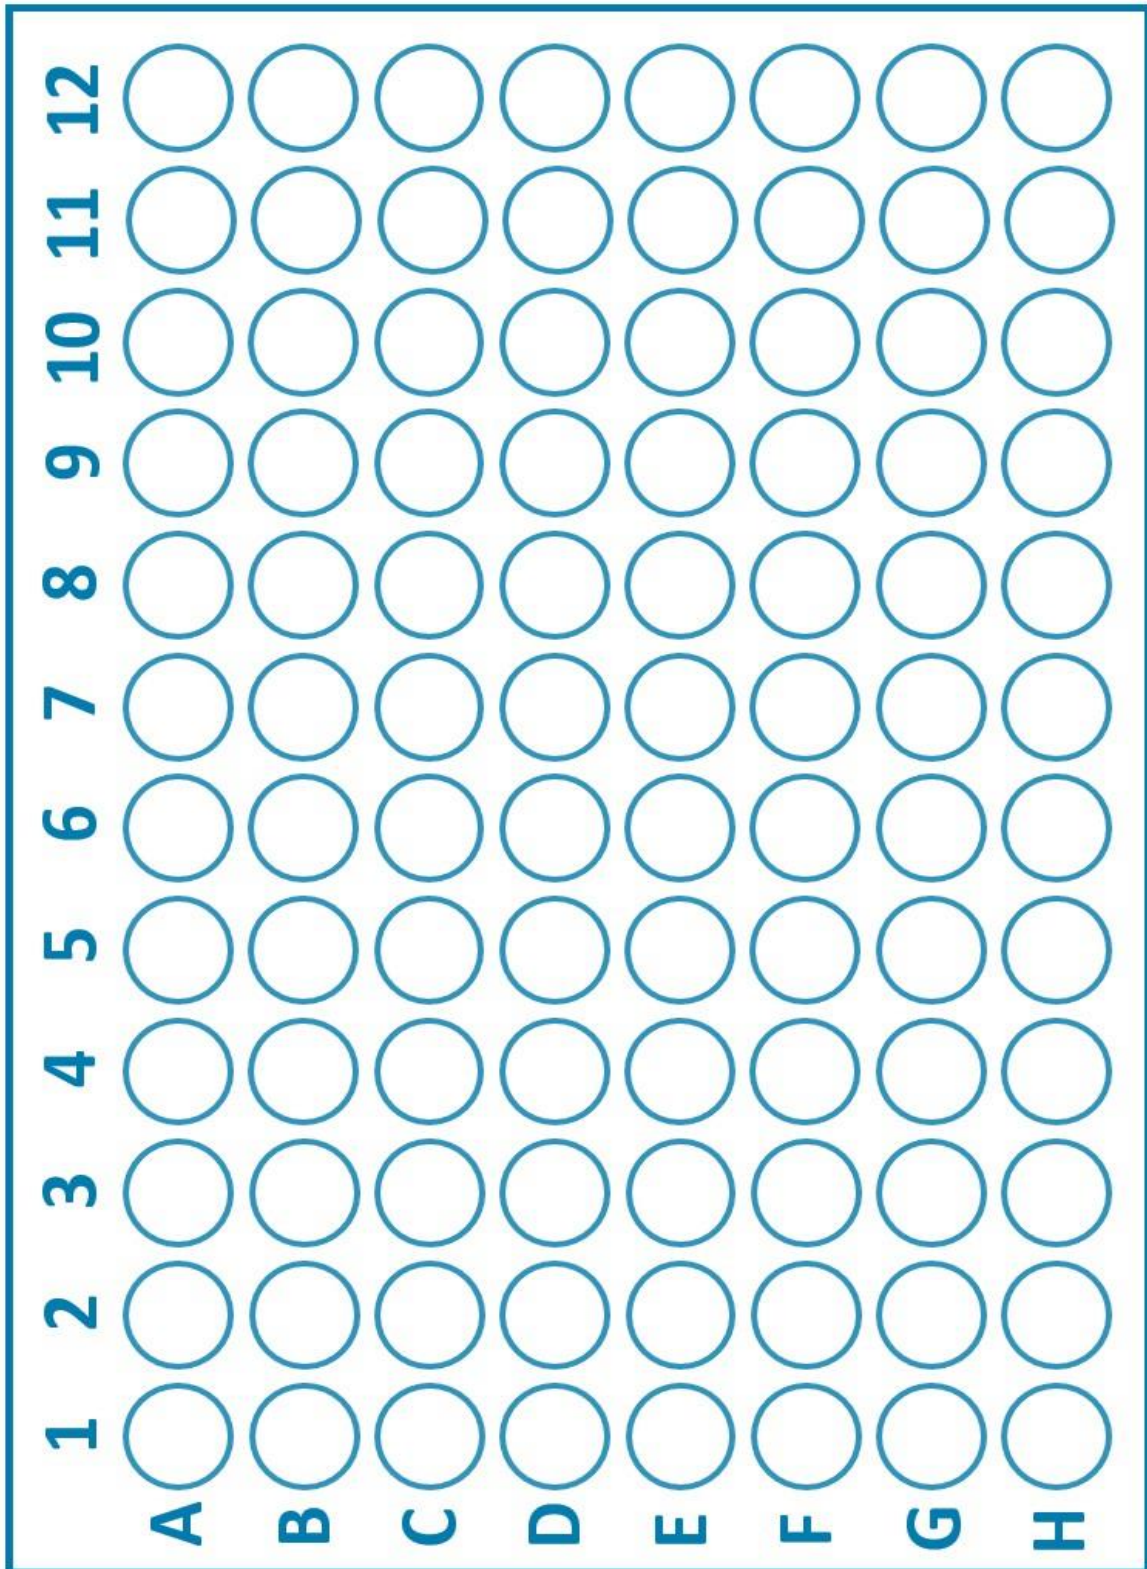



**Figure 2. Multiparametric analysis of cardiac contraction with the FLEXcyte 96 device and FLX-96 plates**

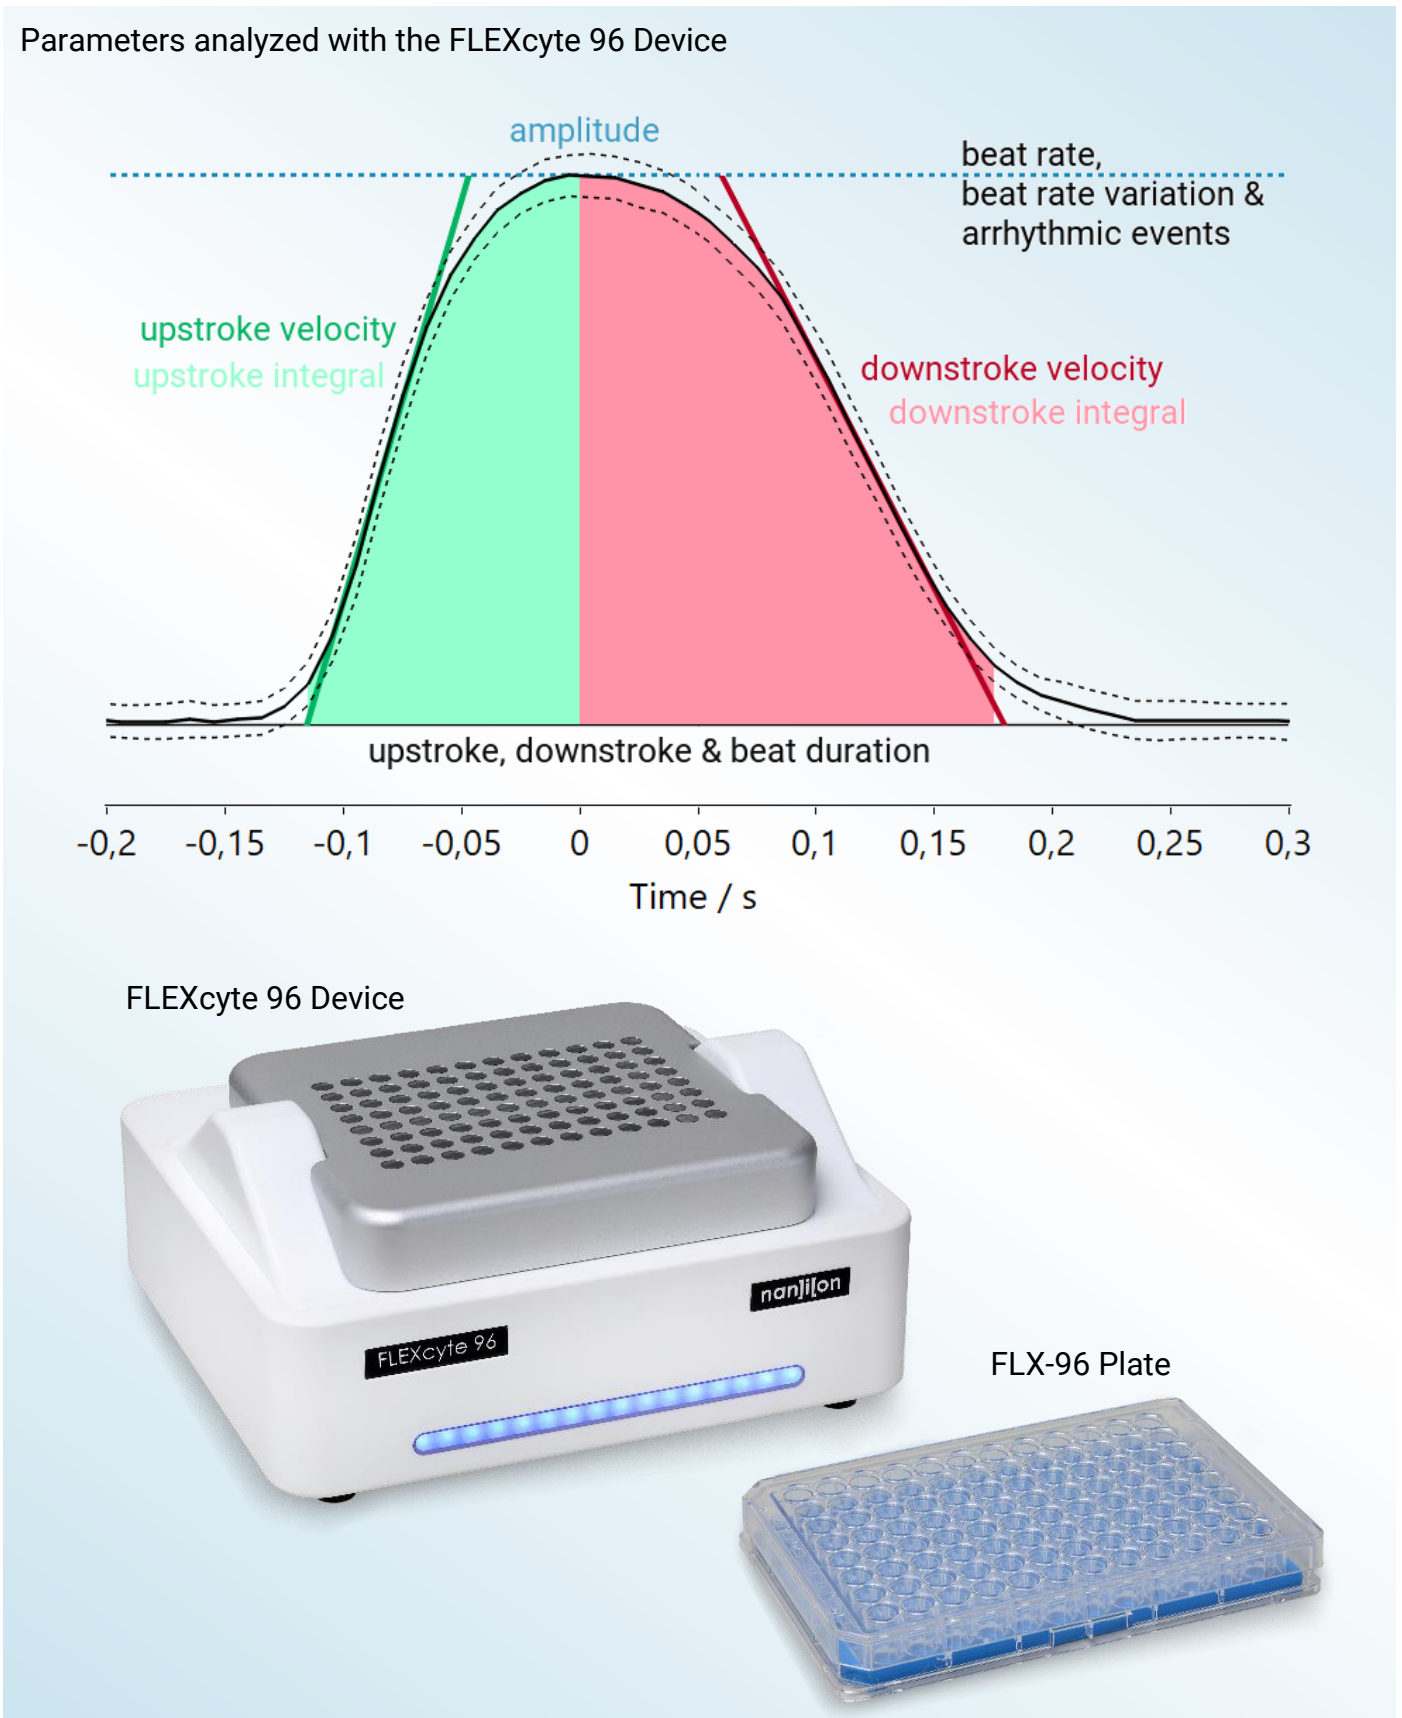









**innoVitro GmbH**  
Artilleriestraße 2  
52428 Jülich  
Germany

**FON** +49 (0) 2461 3170561  
**FAX** +49 (0) 2461 3173859  
**E-MAIL** [info@innovitro.de](mailto:info@innovitro.de)  
**Web** [www.innovitro.de](http://www.innovitro.de)

**inno****vitro**